


CERTIFICATE OF ANALYSIS
Aflatoxin G1 in Acetonitrile LCMS grade

This document is designed, and the certified values and uncertainty are determined in accordance with ISO Guide 31, ISO Guide 34, ISO Guide 35, AOAC, and Eurachem/ CITAC Guides.

Description of the Reference Material (RM)

	Product name:	Aflatoxin G1		
	Product number:	FIA000200		
	CAS number:	Aflatoxin G1	1165-39-5	
	Lot number:	AFG117030702		
	Expiry date:	6-Mar-2025		
	Certified value (s):	Aflatoxin G1	2,00 ± 0,01	µg/mL
	Physical description:	Clear solution of toxin in Acetonitrile LCMS grade		
	Packing	Amber glass vial filled with 1 mL of solution		
	Storage conditions	≤ -10°C		
	Matrix and starting material:	This material was prepared with/from:		
	Acetonitrile UPLC/MS	Batch:	1204102BS	
	Aflatoxin G1	Internal ID:	SS-AFG1-P-14102201	

Intended use of the RM:

For laboratory use for R&D purposes only. The main purpose of this material is for analytical instrument calibration (e. g. external calibration, standard addition). Not for drug, household or other uses.

Instruction for the correct use of the RM:

The vial should be stored in a dark place at ≤ -10°C . Before usage of the RM, allow the vial to warm to room temperature. The expiry date of this RM is based on the current knowledge and holds only for proper storage conditions in the originally closed vials / packages. Solutions prepared for calibration purpose should be protected from exposure to light. Discard solutions after use in accordance with appropriate safety regulations for chemical substances.

Hazardous situation:

H225 : Flammable liquid - Category 2 - Highly flammable liquid and vapour
 H302 : Acute toxicity - Oral - Category 4 - Harmful if swallowed
 H312 : Acute toxicity - Dermal - Category 4 - Harmful in contact with skin
 H319 : Eye irritation - Category 2 - Causes serious eye irritation
 H332 : Acute toxicity - Inhalation - Category 4 - Harmful if inhaled

In case of accident or if you feel unwell, seek medical advice immediately (show the label where possible). Avoid exposure. Wear suitable protective clothing.

Safety measures:

Further information is available in the MSDS provided along with this certificate. Final users should make their own investigations to determine the suitability of the information for their particular research purposes. In no event the supplier of this RM shall be held liable for any damage resulting from handling or from contact with the product.

Traceability

The certified values are based on the results of analytical techniques previously used for purity assessment of solid mycotoxins. High purity material represents a practical realization of concentration units, through conversion of mass to molar quantity.

Calculation of certified values and associated uncertainties

This calibrant is certified on solution preparation. Toxin is pipetted and diluted in Acetonitrile LCMS grade. Mass concentration calculation is based on certified concentration, purity and dilution step.

The pipet was calibrated with traceability to national and international standards (Dakks & ilac-MRA). All weights used for metrological control are connected to national and international standards. The weights are calibrated by an accredited laboratory.

$$C (\mu\text{g/mL}) = \frac{m \times P}{V}$$

Toxin	Source				Standard uncertainty
Aflatoxin G1	Purity		100,00	%	100,00
	Liquid solution	concentration	134,00	$\mu\text{g/mL}$	0,03
	Volumetry procedure	volume	0,30	mL	0,00
	Dilution	volume	20,00	mL	2,00
$Combined_u = \sqrt{\left(\frac{u_p}{P}\right)^2 + \left(\frac{u_{cm}}{V_{cm}}\right)^2 + \left(\frac{u_{vp}}{V_p}\right)^2 + \left(\frac{u_{v1}}{V_1}\right)^2}$					0,01
$Concentration_{Toxin} = \frac{Concentration\ mother}{V_{D1}} \quad \mu\text{g/mL}$					2,00
Total expanded uncertainty (using a coverage factor k=2)					0,01

Notes: The purity of the mycotoxin used for this RM was determined by liquid chromatography. Following the Guide to the Expression of Uncertainty in measurement (GUM) the expanded uncertainty of toxin level is obtained by multiplication with a coverage factor K for which 2 is usually chosen to obtain a confidence level of 95 %.

Quality control


Confirmation of the certified concentration by HPLC-FLD & cell

The certified concentrations of the prepared solution was confirmed by HPLC-FLD & cell against a reference batch.

Chromatogram

Chromatographic conditions:

Column:	InertSustain C18 250 x 4,6 mm5 μm		
Mobile phase:	MeOH / H2O + HNO3 +KBr		
Flow mL/min:	1,80		
Temperature °C:	50,00		
Detector	FLD with post-column electrochemical with bromide using FARLIB® ECD Cell		
Aflatoxin G1	2,02	\pm 0,02	$\mu\text{g/mL}$
Mean of 5 replicates measurement against reference batch, confidence interval with P = 95%			

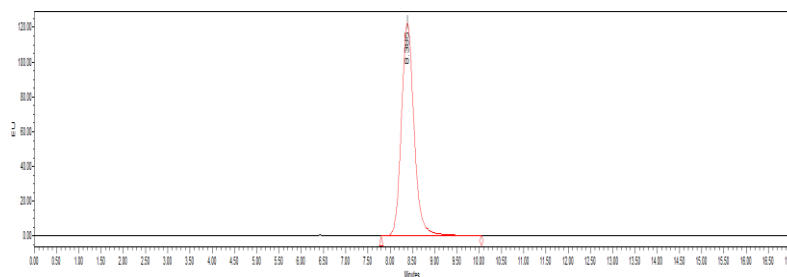

Chromatogram of Toxins

References:

- a-ISO GUIDE 31:2015, Reference Materials - Contents of certificates, labels and accompanying documentation.
- b-ISO GUIDE 34:2009, General requirements for the competence of reference material producers
- c-ISO GUIDE 35:2006, Reference materials - General and Statistical Principles.
- d-ISO/IEC Guide 98-3:2008 Uncertainty of measurement-Part 3 : Guide to the expression of uncertainty in measurement (GUM:1995)
- e-Eurachem/CITAC guide (2019), Traceability in Chemical Measurement.
- f-Eurachem/CITAC guide (2012), Quantifying Uncertainty in Analytical Measurement.
- g-AOAC Official Method 970.44-1971 - Preparation of Standards for Mycotoxins.

This document was computer generated and is valid without signature

Prepared by: Alexandre CLERMONT
Quality Control

Date: 13-Feb-24